

ECOTROC® ET-C
Operating manual
Dewpoint controll device
Rev. 0616-03



Contents

- Contents 2**
- 1. General information..... 3**
- 2. Warranties 3**
- 3. Safety notes 4**
- 4. Symbols used 5**
- 5. Intended purpose 5**
 - 5.1 Intended use 6
- 6. Technical data..... 7**
 - 6.1 Pressure dewpoint sensor7
 - 6.2 Controller 8
- 7. Electrical connection 8**
- 8. Explanations of key functions..... 9**
- 9. Display layout 10**
- 10. Main menu 11**
- 11. System settings 12**
 - 11.1 Software version 12
 - 11.2 Change language..... 12
 - 11.2 Set date and time 12
- 11.3 Display settings 13**
 - 11.4 Key sounds..... 14
 - 11.5 Change password 14
 - 11.6 Restore factory setting..... 15
- 12. Operating mode..... 15**
- 13. Settings after a restart 15**
- 14. Cycle times 17**
- 15. Setting the pressure dewpoint 17**
- 16. Compressor synchronisation 19**
- 17. Alarm reaction 21**
 - 17.1 Optical alarm release (LED) 21
 - 17.2 Acoustic alarm release (buzzer) 21
 - 17.3 Potential-free alarm release (relay)..... 22
- 18. Alarm values and times for pressure dewpoint 22**
- 19. Maintenance settings..... 24**
- 20. Reading out errors..... 25**
- 21. Using password-protected areas 26**
- 22. EC Declaration of conformity 27**

1. General information

Please read this documentation before taking any installation or operational steps.

Having the basic knowledge of this manual is a prerequisite for carrying out programming steps and the daily use of this controller.

Incorrect use or lack of know-how in the *ECOTROConomy*[®] program can cause damage to some parts and affect the operation of the adsorption dryer.

In principle, only instructed personnel or experts should be able to access the password-protected area. This also applies in the event of an alarm. There is a reason why an alarm is triggered and this must be analysed and rectified. Expertise in the field of compressed air is therefore a prerequisite!

Never switch the controller off completely, not even when an alarm is triggered, otherwise the dryer will only pass over a desiccant bed. Over time this has a negative effect on the compressed air values!!!

2. Warranties

For the conditions necessary for compliance with the warranty, please refer to our "General Terms of Sale and Delivery"

The warranty shall be void if:

- The controller is used for anything other than its intended use.
- The instructions in this operating manual are not observed.
- External influences (e.g. incorrect supply voltage, short circuit, etc.) cause damage to the controller.
- Damage is caused because an incorrect tool has been used.
- Damage is caused due to incorrect or faulty installation.
- The controller is used even though defects are evident.
- An unfavourable or incorrect installation is selected.
- The performance data on the type plate is disregarded.
- Damage occurs after installation completed by unqualified personnel.
- Fundamental demands on the electrical work are disregarded.

3. Safety notes



Failure to observe the safety notes can cause physical injuries and damage to the controller or adsorption dryer. Please observe not only the instructions in this operating manual but also the general applicable safety and accident prevention regulations!

1. The *ECOTROConomy*[®] controller may only be operated and serviced after this operating manual has been read.
2. The *ECOTROConomy*[®] controller may only be used for its intended purpose, as described in this operating manual.
3. The operator must ensure that only instructed and authorized personnel operate the *ECOTROConomy*[®] controller.
4. Only suitably instructed and qualified expert staff may carry out maintenance and repair work.
5. The *ECOTROConomy*[®] controller must only be used in an operationally safe state.
 - a. Operating instructions must be visible on the device.
 - b. Any use of the *ECOTROConomy*[®] controller in conjunction with other system components must comply with the performance data.
 - c. Everyone working with the device must know and observe the safety notes.
6. When disassembling parts of the housing and components of the *ECOTROConomy*[®] controller, make sure
 - a. that the mains power plug is disconnected and is protected from restarting.
 - b. that corresponding and suitable tools are used which are designed to be used for electrical purposes.
7. The *ECOTROConomy*[®] controller may only be operated when all components, e.g. following maintenance work, have been refitted and are complete. The housing must also be closed again. Safety devices on the equipment must not be removed or rendered inoperative!
8. The performance data stipulated in this manual must not be exceeded.
9. Alterations and modifications may only be made with the approval from KSI – Filtertechnik GmbH. Unauthorised modifications excludes all liability of any resulting damage.
10. The *ECOTROConomy*[®] controller must not be used if damage is evident or suspected.
11. If strange noises or odours are detected, switch the *ECOTROConomy*[®] controller off immediately.

4. Symbols used

The symbols used in the technical documentation have the following meanings:



Important!

This symbol draws attention to information and tips concerning the correct and economical use of the ETC controller.



Electrical hazard!

This symbol indicates electrical hazards. This work must only be carried out by qualified expert personnel.



General Alert

This symbol marks general safety instructions.



Arrow up!

This symbol is on the "Up" key on the controller.



Arrow down!

This symbol is on the "Down" key on the controller.



OK!

This symbol is on the "Enter" key on the controller.

5. Intended purpose

The controller must only be used to control adsorption dryers manufactured by KSI Filtertechnik GmbH in compressed air systems. It needs a supply of electrical energy.

Using the installed pressure dewpoint sensor, the moisture content is measured directly on the adsorption dryer outlet. The controller then automatically switches the adsorption dryer according to the set pressure dewpoint. This means that fewer cycles are needed for the regeneration, unlike when a time controller is used. This saves energy since regeneration stops once the desired pressure dewpoint has been reached and a cycle only starts after a forced changeover time. (2 cycles an hour instead of 6 cycles).

5.1 Intended use

The controller is exclusively designed to control adsorption dryers manufactured by KSI Filtertechnik GmbH! If the adsorption dryer is used with other manufacturers, this must be agreed with the manufacturer. Other safety guidelines may apply here!

The controller must only be used in the following areas:



- The controller must be installed in a weatherproof location (exposure to sun should be avoided)
- The location must be dry (safety class IP54)
- The location must be frost-free
- The location must be vibration-free
- The location must not be in a potentially explosive atmosphere
- It must be accessible for settings
- It must at best have little dust exposure
- There must be no risk of lightning or other forms of external energy
- It must be free from aggressive or corrosion-promoting substances.



The controller must only be operated within the allowable operating conditions. These are stipulated on the type plate and in this operating manual. Any other use is considered improper and the manufacturer accepts no liability.

The controller must not be converted in any way and its components must not be modified. The use of components other than the original ones from the manufacturer is not permitted, unless this has been agreed with the manufacturer.

For the nominal performance data of the controller, please refer to the Section "Performance data".

6. Technical data

6.1 Pressure dewpoint sensor



| Type of measurement | Specification |
|---------------------------|---|
| Moisture measuring range | - 100° C to + 20° C pressure dewpoint (4-20 mA) |
| Moisture range | 0 – 100 % rF |
| Power consumption | 20 mA (max.) |
| Power supply | 12 to 28 Vdc |
| Pressure range | 0 to 450 bar |
| Accuracy | + - 2% |
| Application temperature | - 40° C to + 60° C |
| Flow rate | For direct use: 0-10 m/s For block fit with outflow: 1-5NI/min |
| Mechanical connection | Screw-in thread 5/8“ UNF with sealing shim |
| Housing material | Stainless steel |
| Dimensions | ∅ 27mm x 132 mm |
| Weight | Ca. 150g |
| Connection | 2-wire power source |
| Protective filter | HDPE filter 10µm |
| EMC immunity | EN 50081 |
| EMC interference emission | EN 50082 |
| Sensor type | Polymer |
| Type of protection | IP66 (NEMA 4) |


6.2 Controller



| Type of measurement | Specification |
|--|---|
| Max. wire cross-section for terminal connections | 1,5 ² |
| Fuse | T3,15A, 250V |
| Power consumption | Max. 3.5 A |
| Power supply | 230 V , 50 Hz |
| Valve outputs | 230 V, 50 Hz |
| Outputs | 1 1 x 4-20 mA (pressure dewpoint) 1 x potential-free alarm output (N/C or N/O) |
| Accuracy | + - 2% |
| Application temperature | - 40°C to + 60°C |
| Flow rate | For direct use: 0-10 m/s For block fit with outflow: 1-5NI/min |
| Housing type | Bopla RCP 170 F |
| Dimensions W x H x D | 166 x 160 x 100 |
| Weight | Ca. 550g |
| EMC immunity | EN 50081 |
| EMC interference emission | EN 50082 |
| Type of protection | IP54 |



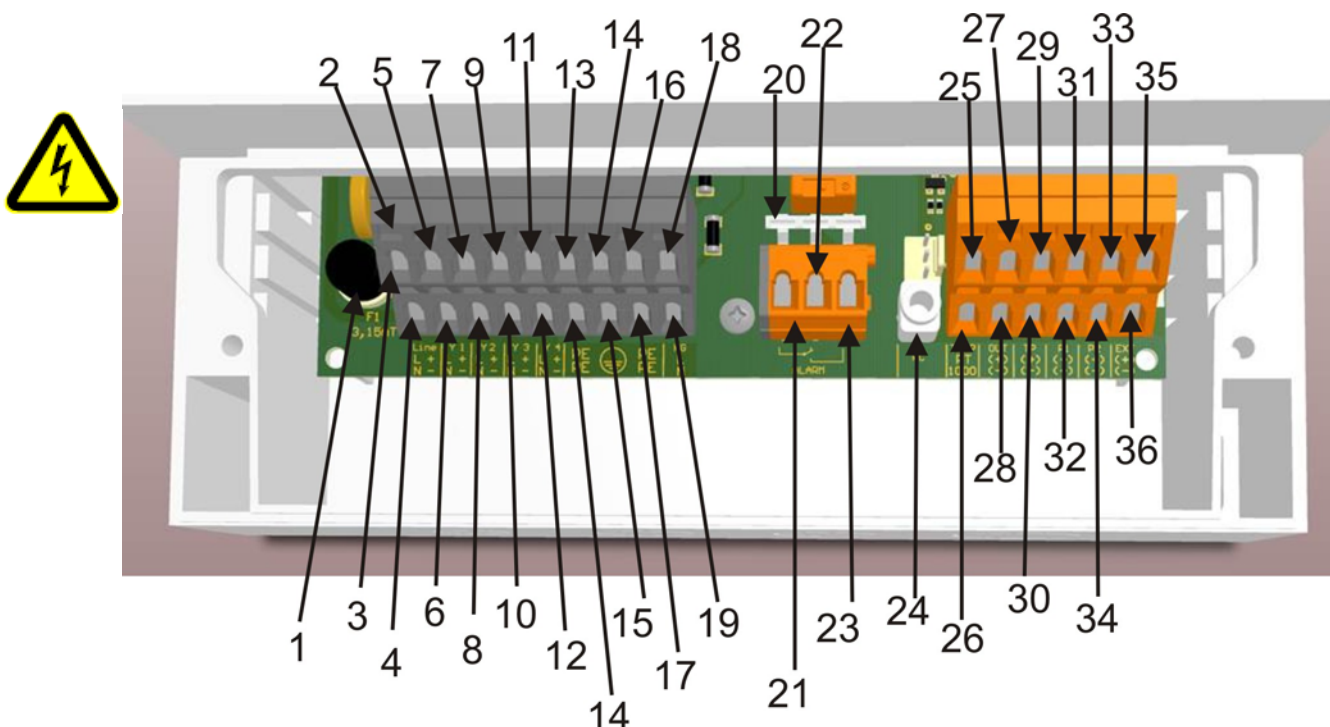



7. Electrical connection

The pin assignment for the controller is as follows:



- | | |
|--|---|
| 1. Fuse F3,5A, 250V | 2. Socket for terminal opening |
| 3. Connection control voltage wire 230V | 4. Neutral wire for control voltage |
| 5. Wire, valve 1 | 6. Neutral wire, valve 1 |
| 7. Wire, valve 2 | 8. Neutral wire, valve 2 |
| 9. Wire, valve 3 | 10. Neutral wire, valve 3 |
| 11. Earthing | 12. Earthing |
| 13. Earthing | 14. Earthing |
| 15. Earthing | 16. Earthing |
| 17. Earthing | 18. compressor synchronisation 230V |
| 19. Neutral wire f.compressor synchronisation | 20. Lever, terminal opening, alarm |
| 21. General alarm | 22. Alarm terminal N/C |
| 23. Alarm terminal N/O | 24. PC connection, jack plug |
| 25. Temperature sensor PT1000 (optional) | 26. Temp. sensor PT1000 (optional) |
| 27. 4-20 mA output + (pressure dewpoint) | 28. 4-20 mA output - (pressure dewp.) |
| 29. Connection, pressure dewpoint sensor + | 30. Connection, pressure dew. sensor - |
| 31. Connection, pressure sensor 1 + (optional) | 32. Connection, pres. sensor 1 - |
| 33. Connection, pres. sensor 2 + (optional) | 34. Connection, pres. sensor 2 - |
| 35. Reserve (optional / not obstructed) | 36. Reserve (optional / not obstructed) |

8. Explanations of key functions

| Image | Designation | Function |
|---|----------------------------|--|
|  | OK key | Use this key to call up the main menu. If you press this key, submenus are displayed. In the Setting menus, this key is used to jump to the next function. When values are changed, press the OK key to confirm them. |
|  | Arrow down key | Use this key to scroll through the menu. Use this key to change values. |
|  | Arrow up key | Use this key to scroll through the menu. Use this key to change values. |
|  | Change values (up or down) | Use this key to change values in both directions |
|  | Power LED | This LED is on when the controller is powered up and is operational. |
|  | Error LED | This LED is on when the controller signals an error (alarm) |

9. Display layout


The display of the ET-C controller offers you the following views and setting options without a password:

The controller powers up when the power supply is connected:




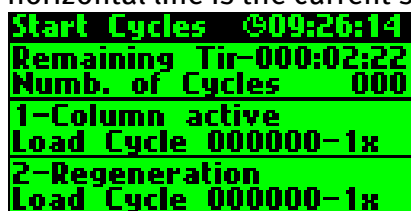
The bottom line shows the software status and the current date.

Once powered up, the measurement of the pressure dewpoint starts. The top line shows the current phase (pressurisation) and time (04:49:42). The time changes with the current date (10.03.00).

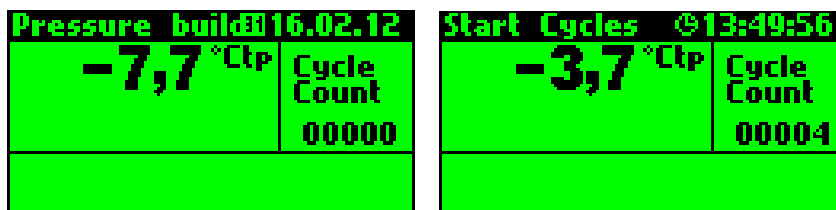

Under Anzahl Zyklen (Number of cycles), all cycles are counted which have been run in the current mode since startup.

Press the  key to go to the second overview page. The first line displays the current phase again and the date changes with the time. Below that, the remaining time of the current status is displayed along with the number of cycles to be completed in the respective mode (in this case, two more cycles in the start cycle). Below the first horizontal line is the current status of the corresponding dryer column.




Once the controller has started up, it may take some time until the desired pressure dewpoint is reached.



Every 15 minutes the display is restarted. This will protect the display against damages through electrical magnetic fields. This process is realized within a quarter second. This is not a mistake, it is a volitionally process.

Depending on the pressure dewpoint value which is set, an alarm is triggered after 2 minutes


which is shown on the display. The first message appears as a piece of information that an alarm / error has occurred and the second message tells you where the alarm / error has occurred.

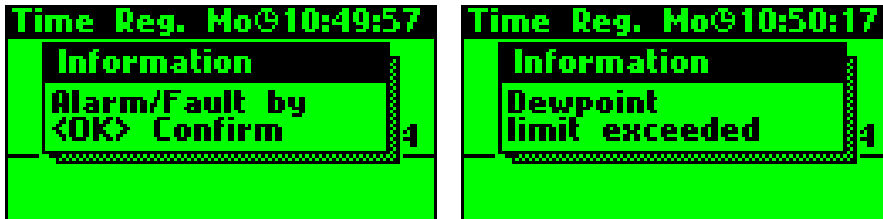

By pressing the **OK** key, you can hide the message for 2 minutes, but the alarm remains in the potential-free output and alarm LED.

10. Main menu

Press the **OK** key to pull up the main menu. The following submenus then appear:

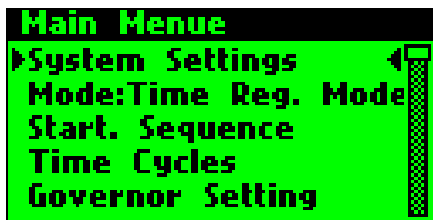

Both triangles in front of and after the respective menu item show you what you have currently selected. Press the **↓** key several times to go to the other submenus.




To return to the overview, press the **OK** key when you have selected "Back". This "Back" command is at the end of every menu.

11. System settings


In the Systems settings menu, you can configure the following settings:



11.1 Software version

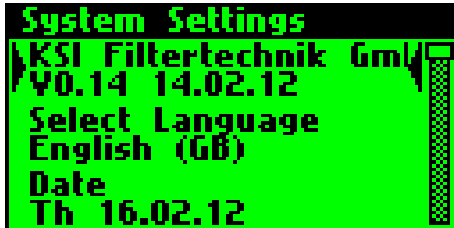

"KSI GmbH" displays the software version and the date of the software.

11.2 Change language


Press the  key to pull up "Select Language".

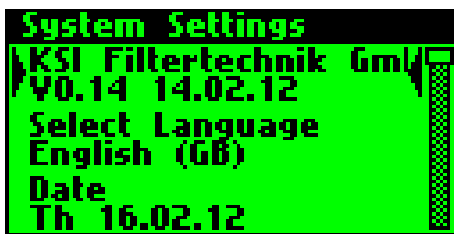


Once these steps have been completed, the language is changed to "English" and you are back in the main menu.

11.2 Set date and time


The controller has a realtime clock. It must be checked, and if necessary set, during commissioning. In order for these entries to appear correctly in the logbook, the date and time are password-protected.

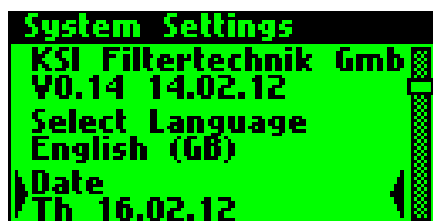

You can only set the date using a password.




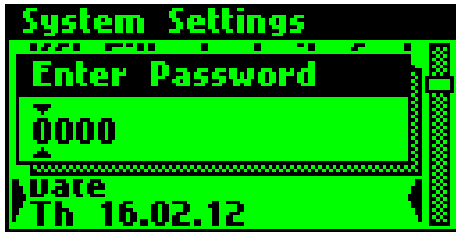


You can only set the time using a password.



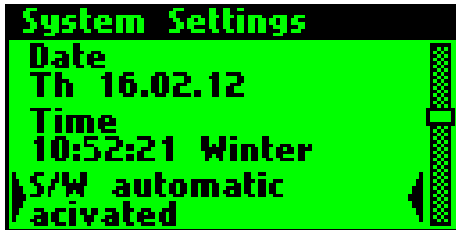


You can only activate / deactivate the automatic changeover of summer to winter time using a password.




11.3 Display settings

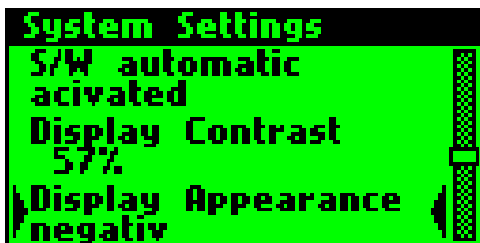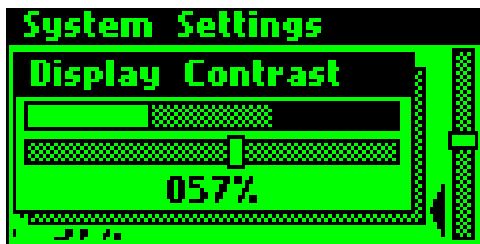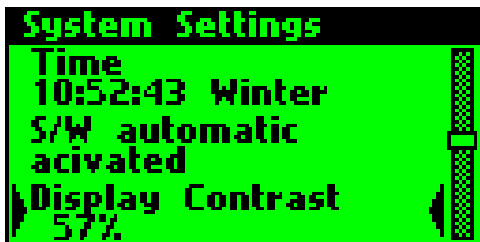

Sets the display to Positive. You are back in the main menu.

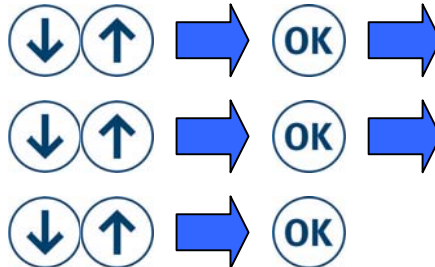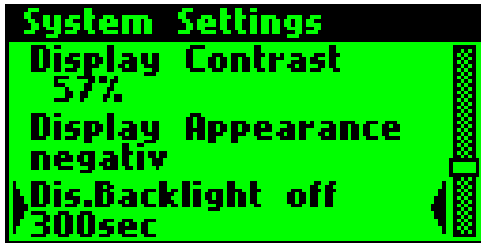


11.4 Key sounds

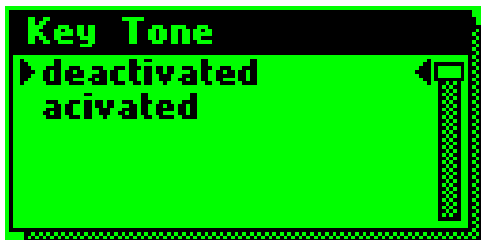

Key sounds are now deactivated. You are back in the Systems settings menu.


11.5 Change password

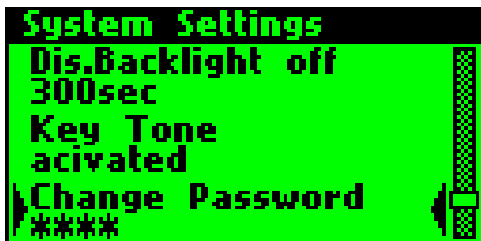


You can only change the password using a password.



11.6 Restore factory setting


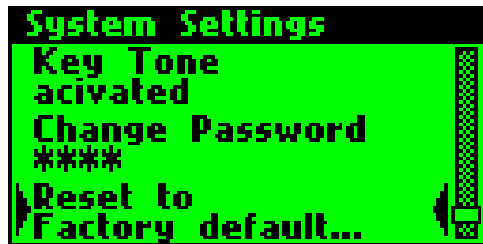


You can only load the factory setting using a password.

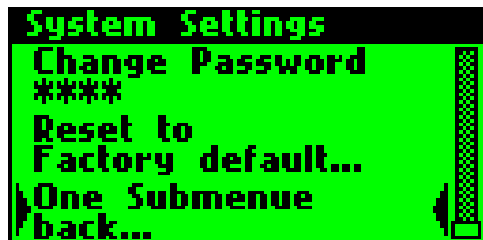


Takes you back to the main menu.




12. Operating mode

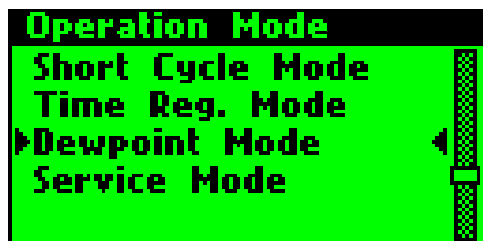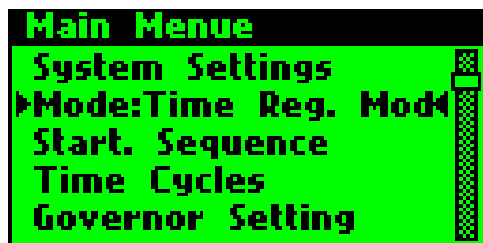




Set the desired operating mode. The password is needed for the Service mode. After you have confirmed the setting, you are taken back to the main menu.

13. Settings after a restart


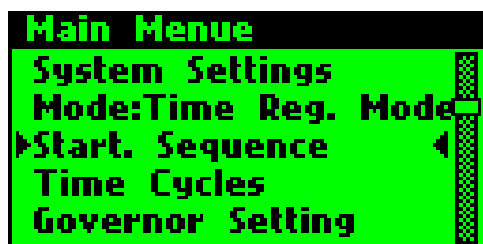


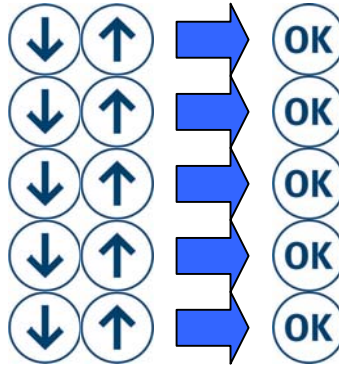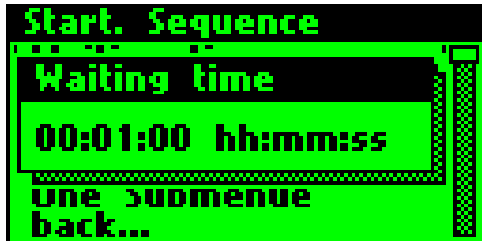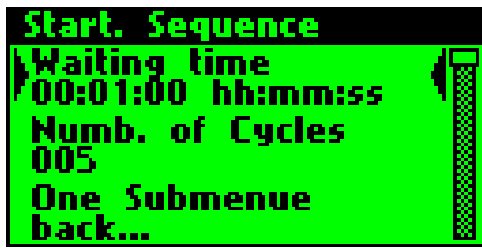

Set the waiting time. After you have entered the last digit, press OK and this takes you back to the "Start sequence" menu.

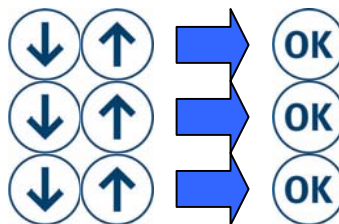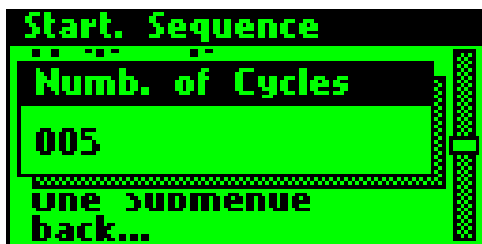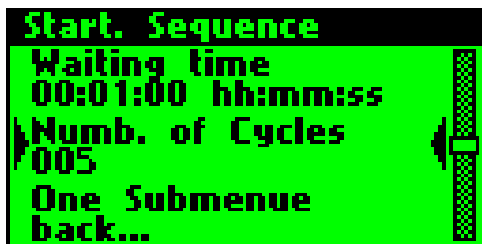


Set the number of short cycles which should be run when the controller is started up.

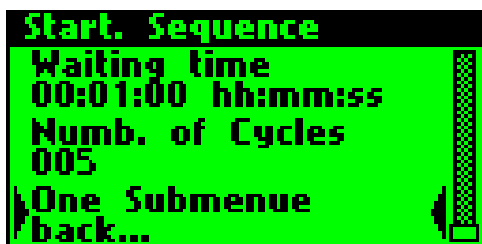


You are back in the main menu again.


14. Cycle times

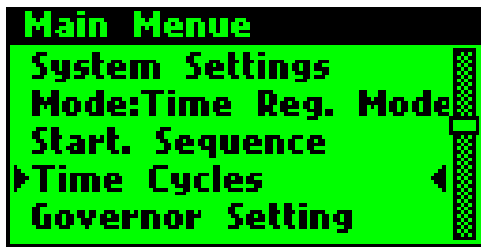

OK

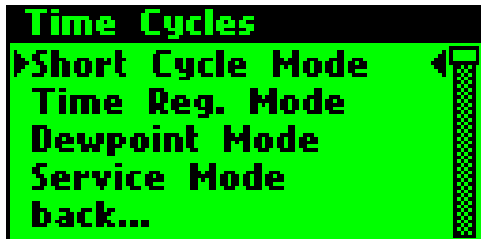


OK

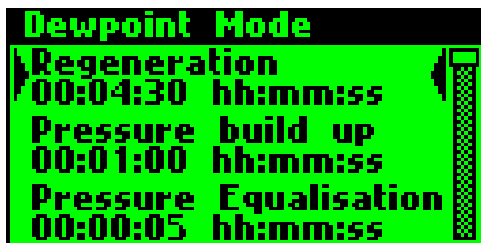

You can only change the cycle times using a password. This applies to all cycle times of the individual operating modes.

15. Setting the pressure dewpoint



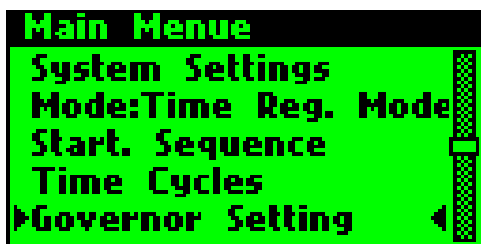


OK



OK

Starting with the software version 1.08 you now can only change this with a password. This is shown below and has to be entered before changing the setting.

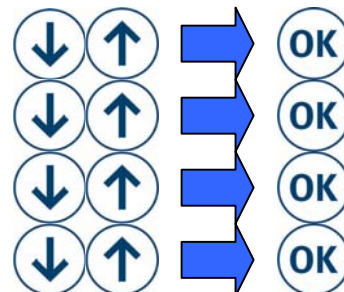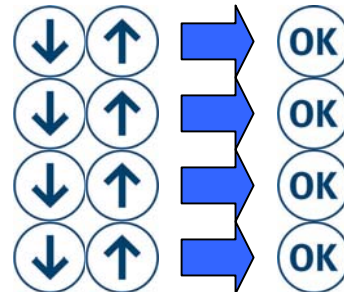
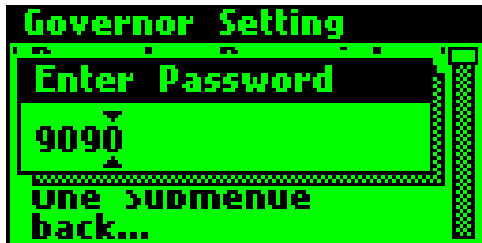


Here, set the pressure dewpoint after which the adsorption dryer should switch to energy saving mode. Please note that the minus can also be converted to plus. Once you have set the last digit and have confirmed the setting by pressing the OK key, you are back in the Control setting menu.

The standard alarm settings will automatically be adjusted to the set "Regular Dewpoint". This applies to the PDP release and the PDP reversal under the menu point "Limit Dewpoint". PDP release will be 2°C and PDP reversal will be 1°C under the set "Regular Dewpoint".




If you wish a different PDP release, for example regular dewpoint -35°C and a DPD release of -20°C this can only be done by your supplier. For this it need the Service-Password.

Please make sure, that by all changes, that are made in the "Governor Setting" you still go conform with the dryer performance. It is not possible to pull down the dewpoint very much, if the dryer was not built for this. If you are not sure, please ask your service partner.

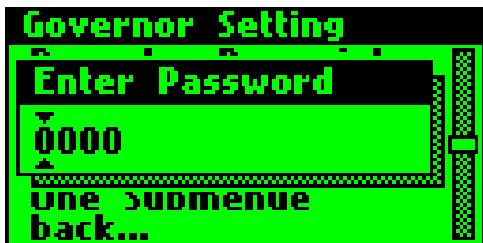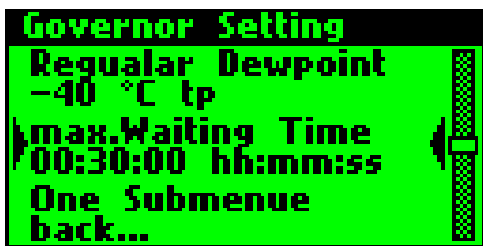



You can only change the stand-by time using a password.

16. Compressor synchronisation

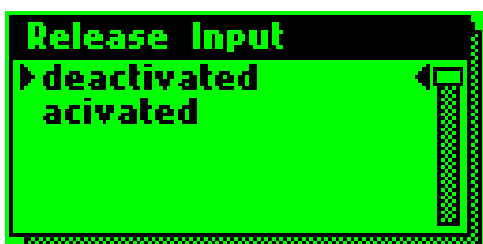
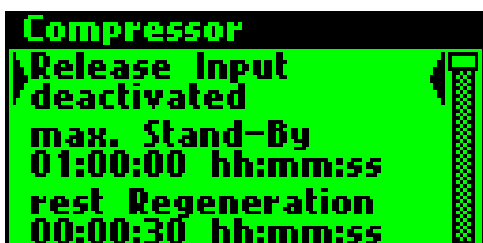
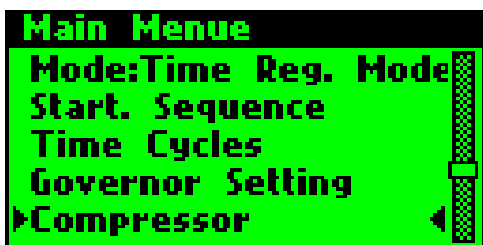


Activate the release input if the controller is to run in the compressor synchronisation. This needs the electrical connection of the compressor to the corresponding control terminal.

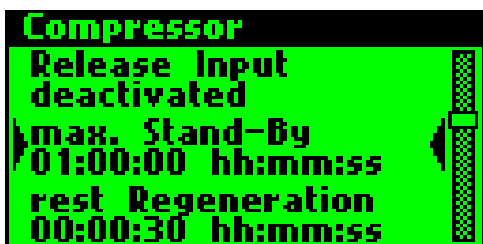

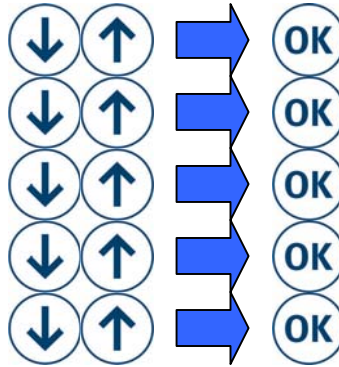


Define the downtime period before a forced changeover takes place. In the example here, the adsorption dryer does not switch for an hour as long as the compressor has not been running during this time. After an hour, the adsorption dryer runs a cycle.

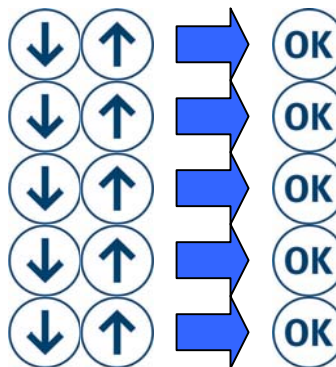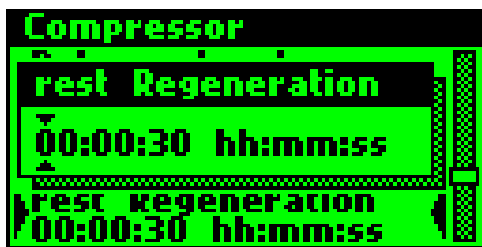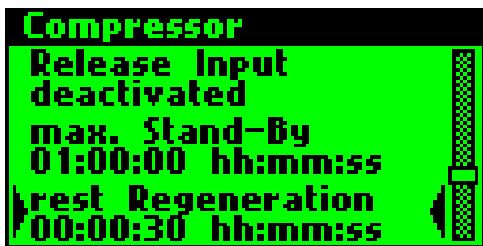


If the compressor does not switch off whilst the last 30 seconds of regeneration are running, this cycle runs to the end. Only then does the adsorption dryer switch to stand-by.



17. Alarm reaction

Error messages can be issued in different ways on the controller. These alarms can be issued as:


- optical signal on the controller via LED 
- acoustic signal from the controller via a buzzer
- switched to an N/C or N/O alarm contact

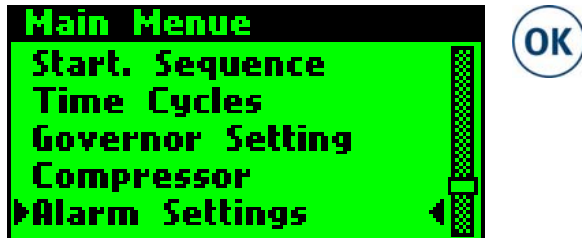

17.1 Optical alarm release (LED)

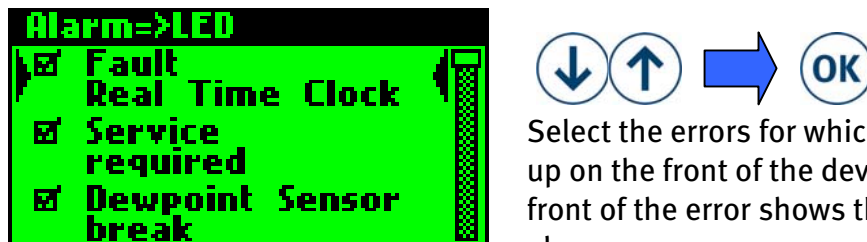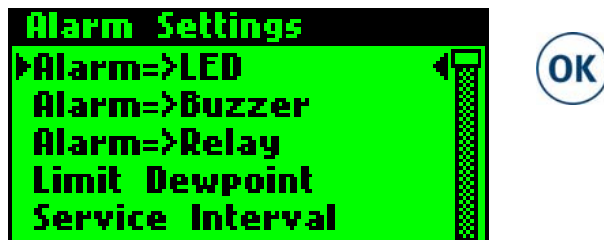



Select the errors for which the LED should light up on the front of the device. The checkmark in front of the error shows the activation of the alarm.

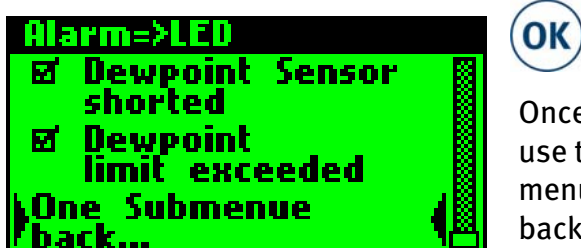


Once you have set all the alarms you want to set, use the arrow keys to return to the displayed menu items. Confirm with OK and this takes you back to the Alarm reaction menu.

17.2 Acoustic alarm release (buzzer)

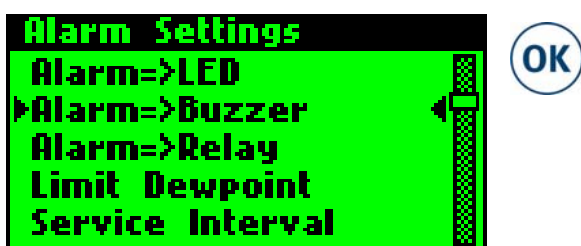


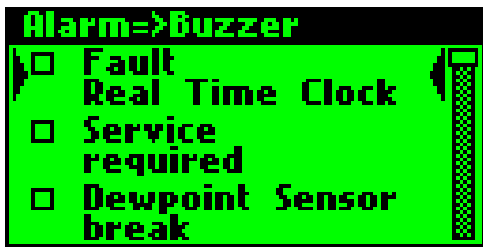


Select the errors for which an acoustic alarm should be emitted. The checkmark in front of the error shows the activation of the alarm.

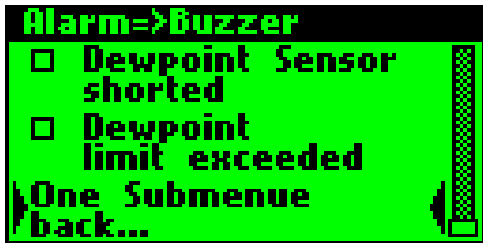



Once you have set all the alarms you want to set, use the arrow keys to return to the displayed menu items. Confirm with OK and this takes you back to the Alarm reaction menu.

17.3 Potential-free alarm release (relay)

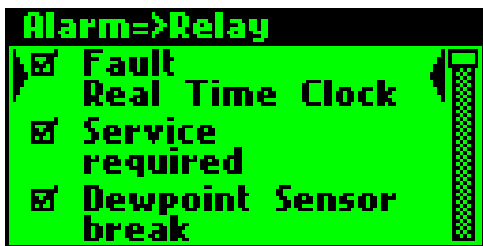
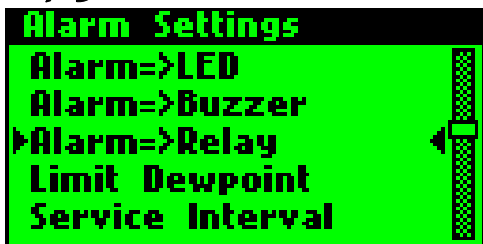


Once you've set all the alarms you want, use the arrow keys to return to the displayed menu items. Confirm with OK and this takes you back to the Alarm reaction menu.

18. Alarm values and times for pressure dewpoint

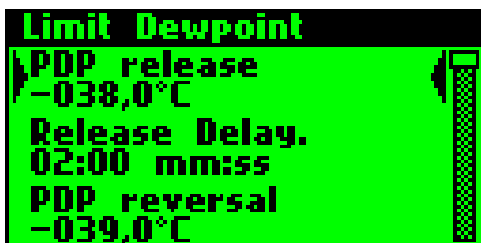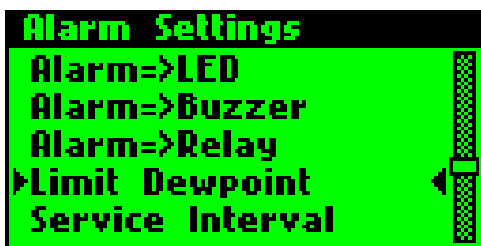



Here, define the pressure dewpoint after which the controller should emit an alarm.

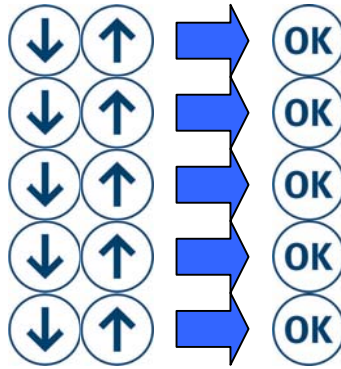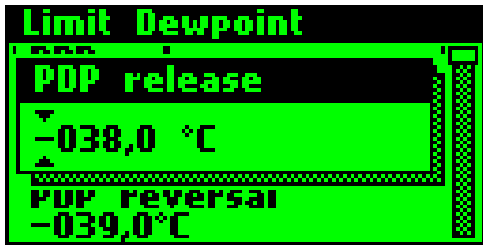



When setting the desired pressure dewpoint alarm value, make sure that the first digit remains a minus. Otherwise the alarm is only triggered at +38°C pressure dewpoint.




To buffer any possible dewpoints peaks, you have the option here to set an alarm delay. The alarm is then only triggered if it is present for longer than the set time.

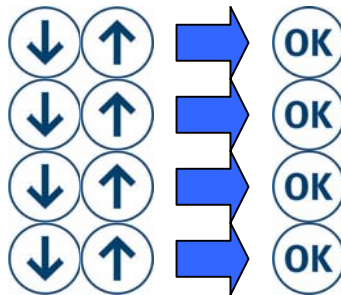
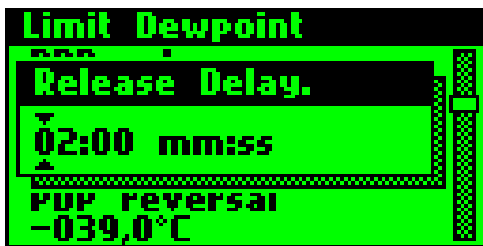


This value must always be higher than the value of the TP trigger. It defines the value when the triggered alarm is automatically reset.

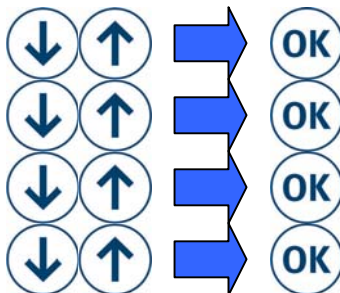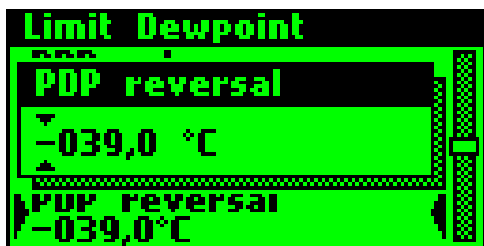


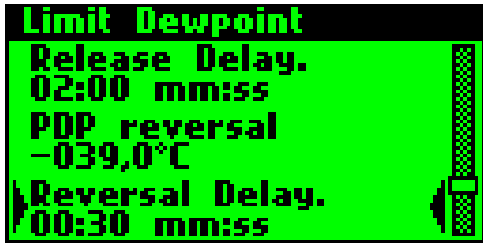

OK

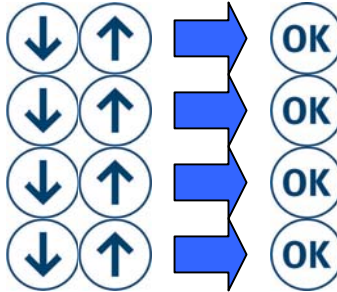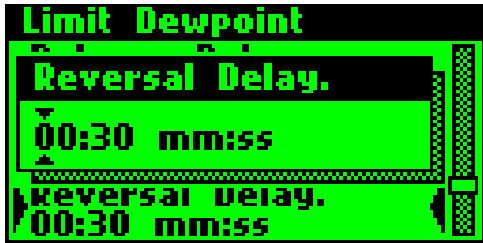


This time defines the period during which the alarm may still be present, after which the values are better again than had been set for the TP cancellation.

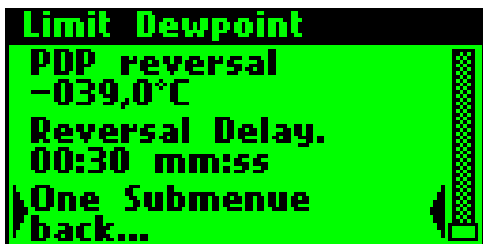


OK

Once you have set all the settings you want, use the arrow keys to return to the displayed menu items. Confirm with OK and this takes you back to the Alarm reaction menu.

19. Maintenance settings

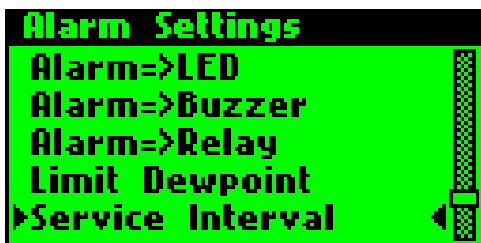

OK

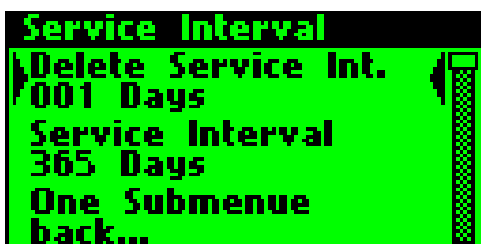


OK


The operating hours are displayed here. The screen on the left shows that there are still 364 days left until the next maintenance.




You can only reset it after the maintenance using a password.

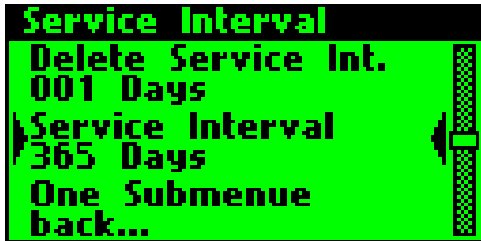

Here, define the time until the maintenance alarm is triggered.

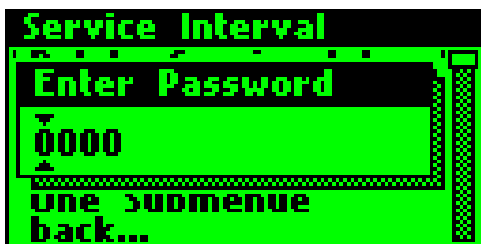


These settings can only be made using a password.

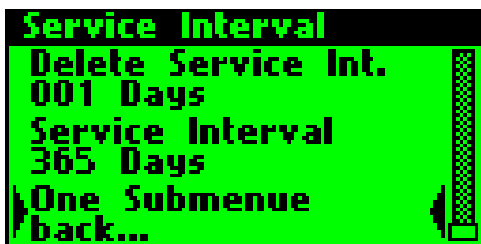

Once you have configured all the settings, use the arrow keys to return to the displayed menu item. Confirm with OK and this takes you back to the Alarm reaction menu.

20. Reading out errors

The ET-C controller records all error values. It also records changes to the settings. This error memory can hold 4000 entries. If all 4000 entries are logged, the oldest entry is overwritten.

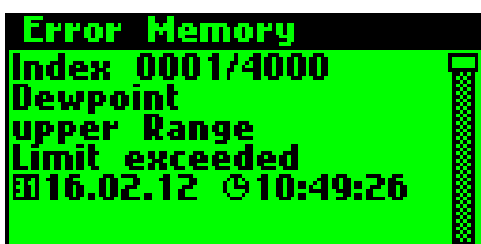

Press the OK key to return to the "Main menu".



Press the OK key to return to the overview.

21. Using password-protected areas



In principle, all changes to the controller settings should be carefully considered. If setting values are incorrectly interpreted or if changes are made without considering the changeover effect, this may cause damage to the adsorption dryer, downstream system components, or products.

The most relevant menu items here are protected by a password and can only be changed by the service technician.

This also protects publicly accessible systems against settings being changed on purpose and thereby causing damage.

If your service technician gives you the password, make sure you use it wisely. Also remember this when you then want to change the password.

If you have changed the password and forgotten it, you have the option to send this controller back to the manufacturer. The manufacturer has a master password which he can use to make the controller accessible again.

22. EC Declaration of conformity

EC Declaration of conformity

We, the authorised representative,

KSI Filtertechnik GmbH
Siemensring 54-56
D-47877 Willich

hereby declare that for the products listed below:

ET-C (ECOTROconomy Comfort) and ET-P (ECOTROconomy Premium)

in accordance with the requirements of the guideline

EMC Guideline 89/336/EEC

conforms to the essential protection requirements which are determined in the Council Directive on the approximation of the laws of the Member States relating to the electromagnetic compatibility (89/336/EEC). This declaration applies to all samples which are produced according to the respective production documents.

To assess the product with regard to electromagnetic compatibility, the following standards have been consulted:

EN 61000-6-3 Electromagnetic compatibility; Generic standard. Emission standard for residential, commercial and light-industrial environments

EN 61000-6-1 Electromagnetic compatibility; Immunity for residential, commercial and light-industrial environments

Any modifications made to the equipment which have not been approved by the manufacturer will annul this declaration.

Signed:



Holger Krebs,
Managing Director